



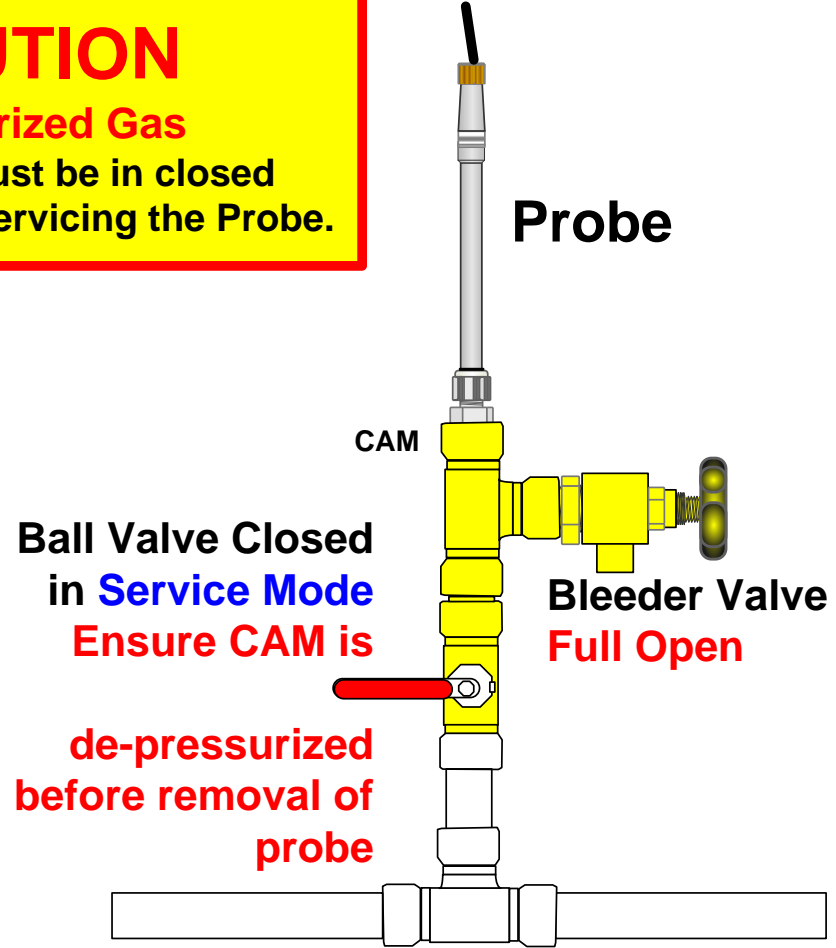

CAUTION
Pressurized Gas
Ball Valve must be in closed position when servicing the Probe.

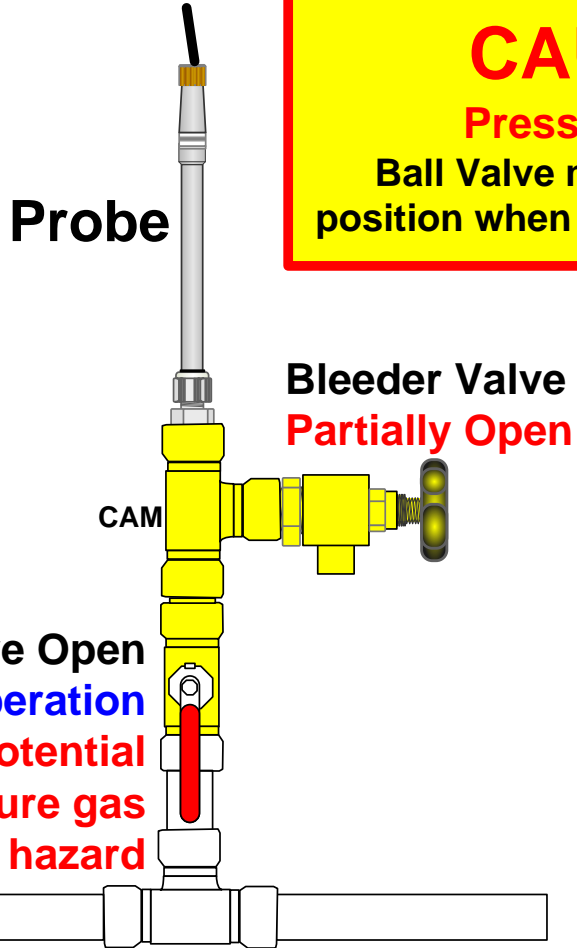

HAZARD WARNING CAM OPERATION		
CAM OPERATION	Reference Only	
	RJN	MARCH 16, 16
Edgetech Instruments Inc.	SK-WL-03162016A	

Reducer Bushing

PROBE

BLEEDER VALVE

TEE

BLEED

CAM

Bleeder Port



BALL VALVE

CAM


Ball Valve Closed

Ball Valve Open


Connection to Compressed Air Header $\frac{3}{4}$ " NPT

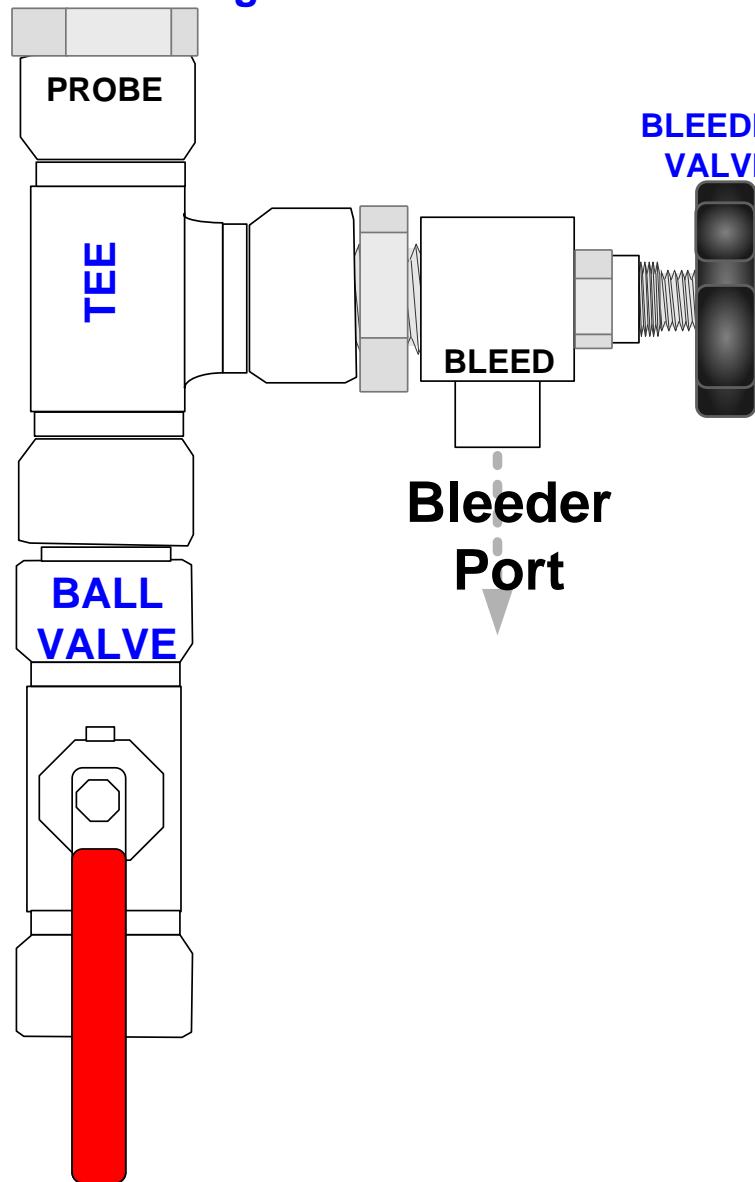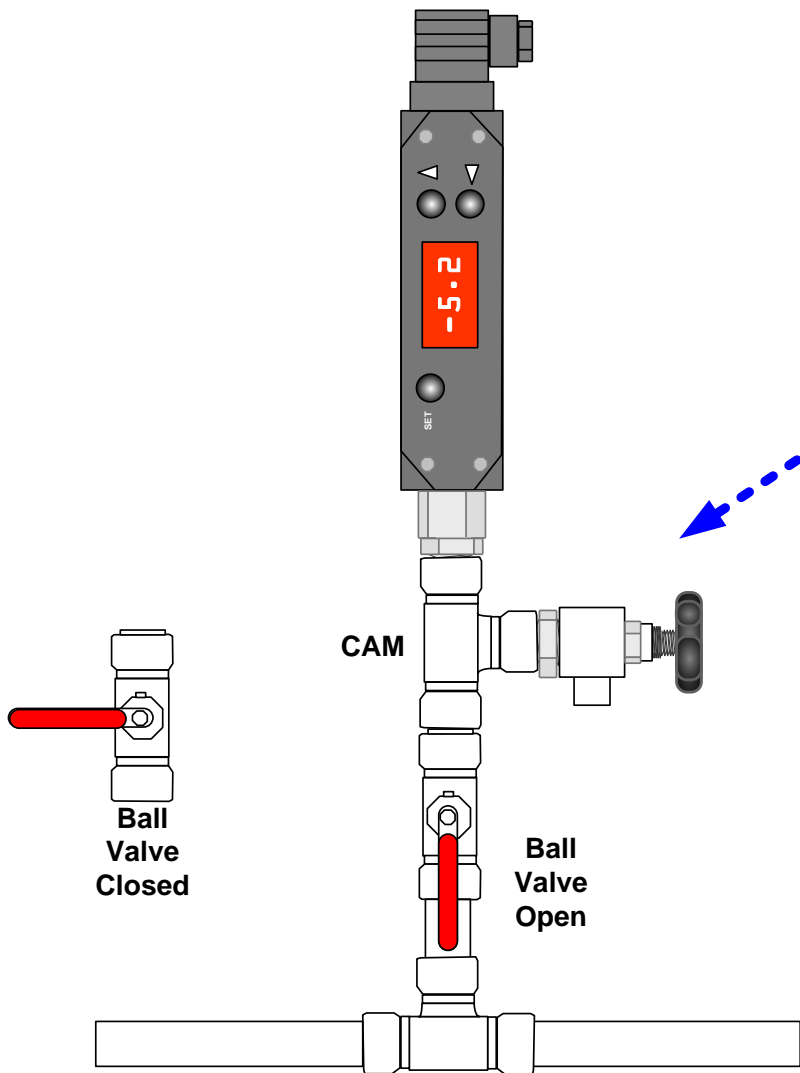

Measuring
Pressure- Dew Point

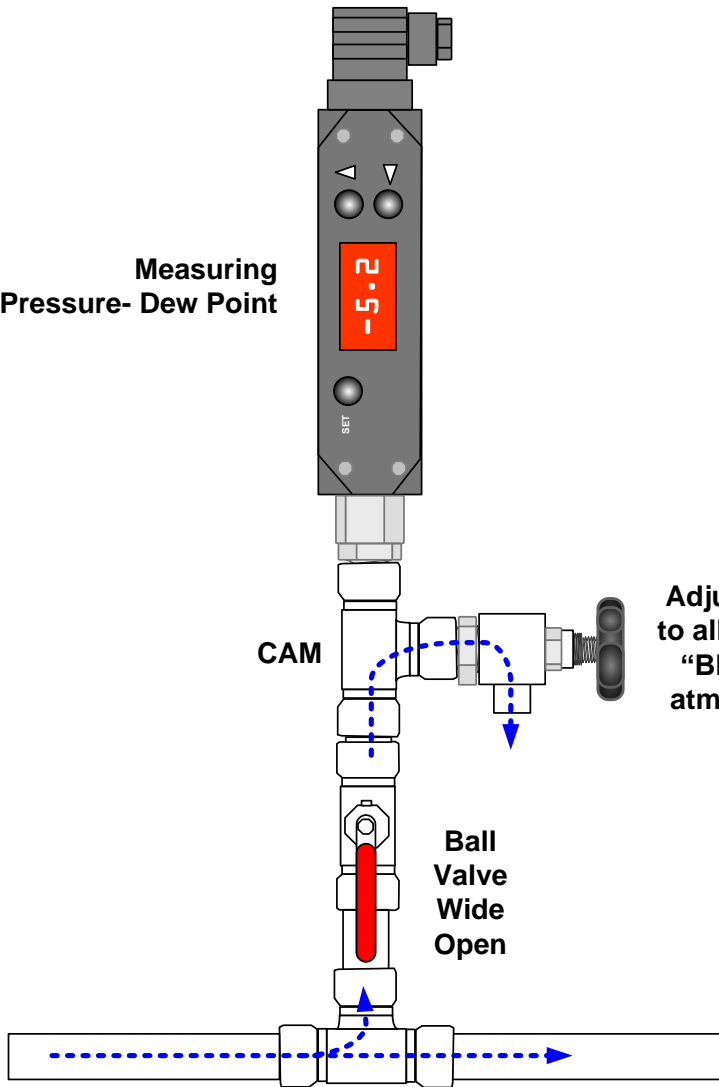

Measuring
Atmospheric Pressure
Dew Point

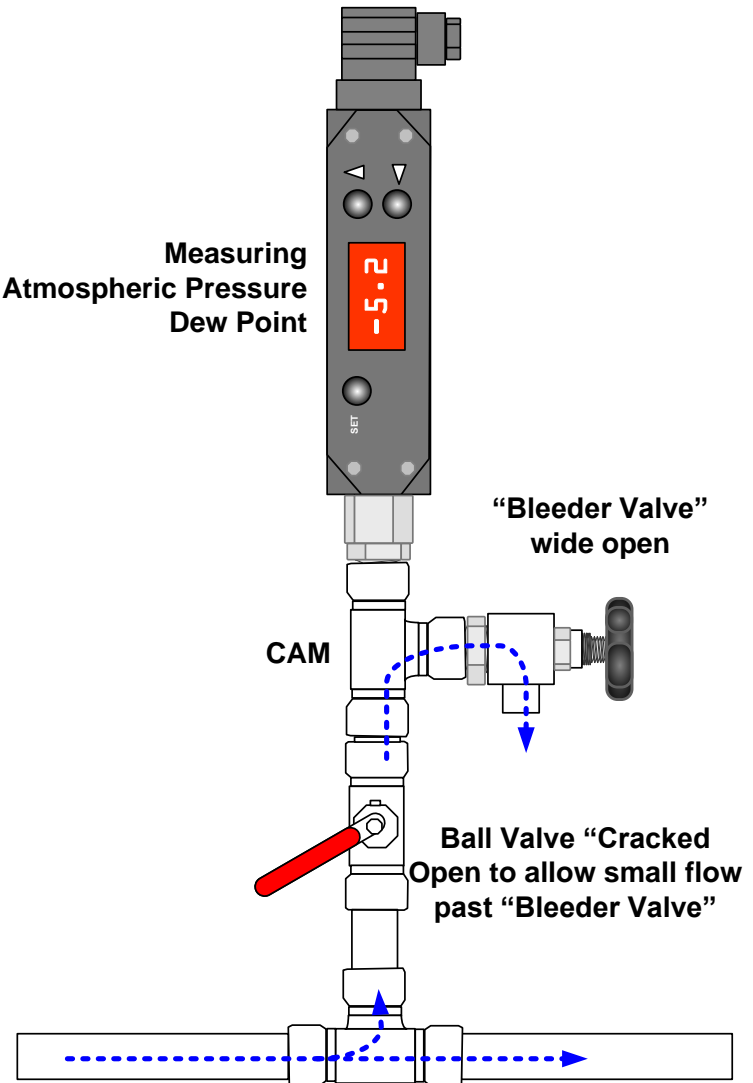

CAM Operation w/ Model 6700 Series Transmitter

CAM OPERATION NOTE	Reference Only	
	RJN	March 16-16
Edgetech Instruments Inc.	SK-O-67-03162016A	